

MD

REF

Applies to the following Models:

EB9060

EB9061

EB9060



EB9061



Important! This User Manual contains important information for the user of the product. All who use this product should review and completely understand its contents. Remember to keep this manual in a place where it is always available to those using the product.

Table of Contents:

Introduction:	2
Safety Precautions & Definitions:	3
Installation & Unpacking:	5
Technical Specifications:	5
Table Operation:	6
Inspection and Preventative Maintenance:	8
Upholstery Cleaning & Care:	8
Service:	9
Replacement Parts:	9
Warranty:	10
Manufacturer Information:	10

Introduction:

The our ErgoBasic just got better...By adding the manual hydraulic pump elevation to this table, we have created a very affordable elevating adjusting table with a pelvic drop. Sleek, elegantly simple, yet still affordable, the ErgoBasic with Manual Pump Elevation offers a critical mix of adjusting features that is praised by many practitioners. A tilt adjustable face headpiece and Accelerator™III pelvic drop come standard. The EB9060 pump elevating Ergo Basic table has a lifting capacity of 400LBS and height range of 18"-24" and the EB9061 pump elevating Ergo Basic table has a lifting capacity of 400LBS and height range of 22"-28". The manual hydraulic pump system eliminates having power cords strung across the floor.

Intended Use: The EB9060 and EB9061 are manually operated tables that can be adjusted to various positions and is used to support a patient during examination and/or treatment.

Safety Precautions & Definitions:



WARNING: Never leave patient on table unattended.



CRUSH HAZARD: Powered components used to elevate and lower this table present a potential crush hazard. KEEP CHILDREN AWAY FROM TREATMENT AREA. Allow only the patient and authorized staff in treatment area.










ELECTRICAL CONNECTION: For your personal safety, this table must be grounded. This table is equipped with a power supply cord having a three (3) prong grounding plug. To minimize possible shock hazard, it must be plugged into a mating three (3) prong grounding type wall receptacles, grounded in accordance with the National Electrical Code and local coded and ordinances. If a mating wall receptacle is not available, it is the responsibility and obligation of the customer to have a properly grounded three (3) prong wall receptacle installed by a qualified electrician. Power requirements of the table are found in the Technical Data Section.

Before using this equipment follow the following safety precautions:

- Before using this equipment make sure you have read and understand this entire manual.
- Explain proper use to all employees. This table should be used only by qualified, trained personnel.
- Never exceed the table's maximum supported weight.
- Use only on dry surfaces. Ensure the tables feet do not slide.
- This table is NOT for patient transport.
- Keep table away from high moisture areas.
- Always explain to the patient how to properly get on and off the table. Be sure to assist patient to prevent falls.
- Keep patient's hands positioned on the top side of cushions at all times.
- Keep hands and feet away from moving parts and pinch points.
- Do not alter the table.
- Never leave patient unattended on table.
- Follow preventative maintenance instructions provided in this manual.
- Ensure all components have been inspected for damage and are fully functional.
- Inspect cables and connectors before each use.
- If you need service assistance contact Pivotal Health Solutions at 1-800-743-7738.

Warning and Precautions through this manual are indicated by specific symbols. Applicable symbols are shown below along with a description of the symbol. Review these symbols and all safety precautions before operating the table.

	CAUTION: Text with a “CAUTION” indicator will explain possible safety infractions that could have the potential to cause injury.
	WARNING: Text with “WARNING” indicator will explain possible safety infractions that will potentially cause serious injury and equipment damage.
	Pinch Point: Indicates space between manually adjustable moving and stationary parts where body parts may become caught, leading to minor injury.
	Crush Hazard: Indicates space between powered moving and stationary parts that represent a potential crush hazard.
	Instructions for Use: Indicates the need for the user to consult the instructions for use.
	Indicates the device manufacturer.
	Indicates the product is a medical device.



WARNING: Under no circumstances should the table be modified from its original design. Contact Pivotal Health Solutions if you need help with service.

Installation & Unpacking:

A MINIMUM OF TWO PEOPLE ARE REQUIRED TO LIFT AND MOVE THE TABLE. LIFT THE TABLE BY THE BASE FRAME!




WARNING: Do not install/use this equipment adjacent to, or stacked with, other equipment as it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify they are operating normally.

After removing the top and side panels of the shipping crate, you may notice metal bands and plastic cable ties. These are used to secure various sections of the table and must be removed. Once all bands and cable ties are removed, the table must be lifted directly upward in order to clear all shipping restraints.

Once the table is out of the shipping crate, place table in a level location and inspect the table cushions, frame, cables, etc. for damage. If no damage is noted, plug in the table and test the elevation, drops, and any other options that are on your table. Contact Pivotal Health Solutions or your dealer with any questions or concerns.

Instructions for Damaged Merchandise: The contents of this shipment have been checked and packed by experienced personnel. If your company arranged the shipping, damage should be noted on the Bill of Lading before signing to accept the shipment, then articles damaged in transit should be reported at once to delivering carrier and a claim must be filed by you. If freight was arranged by Pivotal Health Solutions, note any damage on the Bill of Lading before signing acceptance of product and notify Pivotal Health Solutions right away. Failure to inspect for shipping damage prior to signing for the product may affect your warranty. We can neither be responsible for, nor can we accept the return of merchandise damaged in transit during shipment arranged by outside parties.

Technical Specifications:

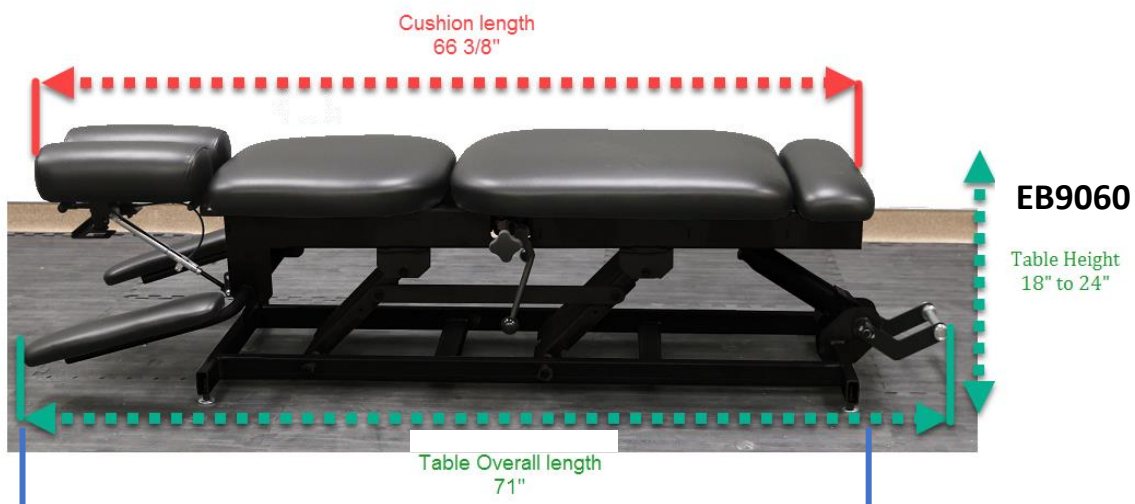

Base Model Number	EB9060	69.5" length	EB9061
Model Name	ErgoBasic with Manual Pump Elevation		ErgoBasic with Manual Pump Elevation
Dimensions	27.25" W x 69.5" L		
Cushion Width	20.5" (widest point on table)		
Height Range	18 - 24" H		22 - 28" H
Foam	Firm		
Lifting Capacity	400 lbs (181 kg)		



WARNING: Keep table out of high moisture areas. For indoor use only.

Operating Conditions: This table should be operated, between 40° F (4.4° C) and 100° F (37.8° C), with relative humidity ranging from 30% - 80%.


Transport & Storage Conditions: This table should be transported and stored in temperatures between -40° C (-40° F) and 70° C (158° F) with relative humidity 10%-100%.

Expected Life: This product has an approximate expected life time of 10 years when correctly handled, serviced, and inspected in accordance with these instructions.

Design and Quality: Pivotal Health Solutions is certified in accordance with ISO 13485, the standard for the medical device industry.

Product Changes: Pivotal Health Solutions, Inc. reserves the right to make products changes without prior notice. Contact your Pivotal Health Solutions representative for advice and information about product upgrades.

Table Operation:

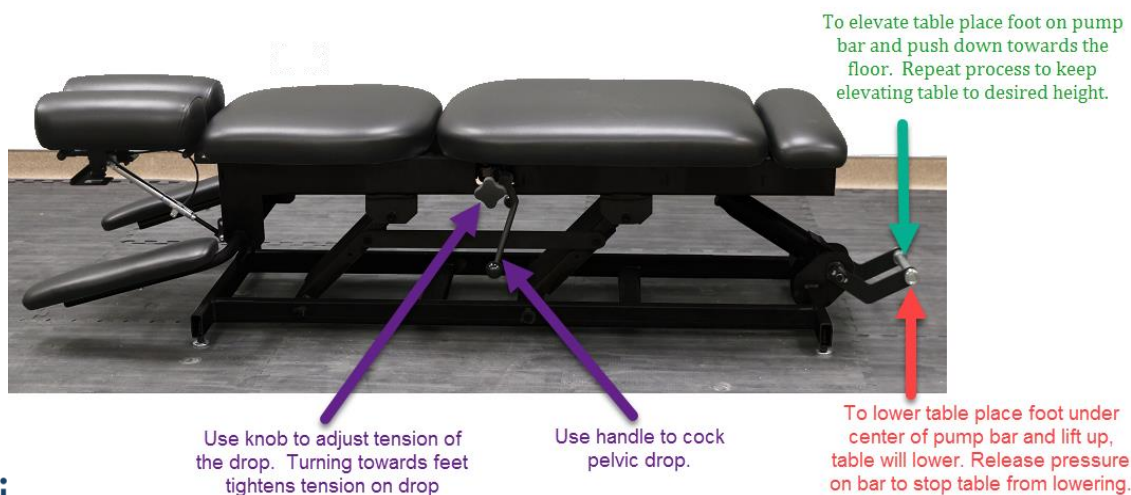



WARNING: Not for patient transport.



CRUSH HAZARD: Powered components used to elevate and lower this table present a potential crush hazard. KEEP CHILDREN AWAY FROM TREATMENT AREA. Allow only the patient and authorized staff in treatment area.



PINCH POINT: Always keep patient's hands positioned on top side of cushions when lowering, raising and tilting table to keep from potential pinch points.

Note to user: If a serious incident occurs, report the incident to Pivotal Health solutions. (See section with Manufacturer Contact Information for contact details). If the incident occurs in the EU, also report any serious incident to the Competent Authority of the Member State in which the user and/or patient is established.

Assisting Patient onto Table:

- 1) The practitioner or trained staff should always assist the patient on the table. Do not allow the patient to get on the table by him/herself.
- 2) The patient should check clothing for keys, wallet, belt, or any other items that may cause discomfort during treatment or damage upholstery.
- 3) Never leave patient unattended while on the table.

Table Operation:

- 1) To begin treatment, position the patient on the table.
- 2) If table is in lowered position, elevate to the desired height for treatment once the patient is in place.
- 3) Perform the treatment desired. Refer to the 'Operation' section and/or the individual component functions below for operation of specific table features.
- 4) After treatment, return the table to a level and straight configuration.

Assisting Patient off of Table:

- 1) Caution the patient not to get up from the table alone so as to prevent any strain that could void the treatment, and to ensure the patient is not lightheaded from lying down which can cause imbalance.
- 2) Allow patient to get full balance before coming to a standing position. Best practice is to keep a hand on the patient at all times.

Inspection and Preventative Maintenance:

INSPECTION:

At least monthly the table should be thoroughly inspected for wear and tear, loose hardware and parts, and other damage.

- Inspect the table to make sure that there is no external damage or loose hardware. Tighten loose hardware. Hardware that does not tighten needs replacement.
- Inspect table for obvious signs of damage or wear such as cracked welds, loose bolts, frayed or damaged cords. Do not use a table with damaged cords.
- Check moveable components (electrical and non-electrical) to ensure functionality.
- Check components to ensure they lock and function properly.
- **Contact Pivotal Health Solutions with questions or concerns.**

LUBRICATION:

- **DO NOT** lubricate friction locks. Lubrication will cause them to fail.

Upholstery Cleaning & Care:



CAUTION: Read carefully, improper cleaning will void the warranty. Never use alcohol-based cleaning agents.

DISINFECTING: There is a disinfecting wipe on the market called *Protex Ultra Disinfectant Wipes*. Many of our customers use these.

FOR DAY TO DAY CLEANING: A solution of 10% mild household liquid dish soap with warm water, applied with soft damp cloth. Rinse with clean water and dry.

FOR STAINS: Dampen a soft white cloth in a one to one (1:1) solution of Fantastik® and water OR Formula 409® and water. Rub gently and rinse with a water dampened cloth.

FOR MORE DIFFICULT STAINS: Dampen a soft white cloth with a solution of household bleach (10% bleach / 90% water). Rub gently and rinse with a water dampened cloth to remove bleach concentration.

WHAT NOT TO USE: Using the wrong cleaning agents you will VOID YOUR WARRANTY and crack, dry out and destroy your vinyl. Do not use any cleaning agents that contain alcohol, harsh chemicals or abrasives.

Service:

Refer to Warranty section in this manual for specific warranty information.

When replacing worn parts, use genuine Pivotal Health Solutions, Inc. parts by contacting our service department. When ordering replacement parts:

- Ask for the service department, 800-743-7738
- Have the model number and serial number available
- Specify parts by the numbers/description below

Technical Information:

Pivotal Health Solutions will make available, upon request, circuit diagrams, component part lists, descriptions, calibration instructions, or other information that will assist service personnel.

Resale or Disposal:

A therapy table is considered a medical device by the Food and Drug Administration. Therefore, it is necessary that Pivotal Health Solutions, Inc. be notified if the table is sold, destroyed, or otherwise disposed of. Please notify in writing providing your name and the serial number of your table to:

Pivotal Health Solutions
Attn: Quality
3003 9th Ave. SW
Watertown, SD 57201

Replacement Parts:

Face Cushion	95038	Hydraulic Pump	60116
Arm Cushion	65454	Pump Bar	60118
Chest Cushion	89489	Pump Handle X2	60115
Pelvic Cushion	89208	Glide Leveler X 4	60007
Ankle Cushion	89205	Head Piece Tilt Mechlock	65471
Pelvic Drop	95544	Knob (Drop Tension Knob)	88282
Lever Actuator (Lift Head Up Down)	95203	Lever Actuator (Head Tilt)	95191

Headpiece	
Standard Head Tilt/Adjustable Cushions	ES95001
Optional Headpiece	
Head Tilt, Forward Drop, Adjustable Cushions	ES95002
Head Tilt, Elevation, Adjustable Cushions	ES95003

Warranty:

Warranty details can be found at: <http://www.phschiropractic.com/customer-service/warranty.aspx>

Note: Warranty periods listed apply only to products purchased in new condition. Any tables sold as a factory blemish or in used condition are sold 'as-is' and are limited to a (1) year warranty on the frame only, commencing on the date of delivery.

Note to user: If a serious incident occurs, report the incident to Pivotal Health solutions. (See section with Manufacturer Contact Information for contact details). If the incident occurs in the EU, also report any serious incident to the Competent Authority of the Member State in which the user and/or patient is established.

Manufacturer Information:

Rev H 10-18-2024



Pivotal Health Solutions, Inc.
3003 9th Ave. SW
Watertown, SD 57201
USA



800-743-7738



011-1-605-753-0110



Fax: 605-882-8398



service@pivotalhealthsolutions.com



www.pivotalhealthsolutions.com



Emergo Europe
Westervoortsedijk 60
6827 AT Arnhem
The Netherlands



Sissel France SAS
14 rue des Grandes Bosses
44220 Couron
France



UK Responsible Person
Emergo Consulting (UK) Limited
Compass House, Vision Park Histon
Cambridge CB24 9BZ
United Kingdom



Performance Health International Ltd.
Nunn Brook Rd, Huthwaite Sutton-Ashfield,
Nottinghamshire NG17 2HU
United Kingdom



MedEnvoy
Gotthardstrasse 28
6302 Zug
Switzerland



Medidor AG
Lenzburgerstrasse 2
CH-5702 Niederlenz
Switzerland